

Cholesterol FS*

Diagnostic reagent for quantitative in vitro determination of cholesterol in serum or plasma on Sysmex BX-Series

Order Information


Cat. No.	Kit size	Number of tests
1 1300 99 10 970	R1 4 x 31.7 mL	BX-3010 4 x 200 tests BX-4000 4 x 154 tests

Method

"CHOD-PAP": enzymatic photometric test

Principle

Determination of cholesterol after enzymatic hydrolysis and oxidation. The colorimetric indicator is quinoneimine which is generated from 4-aminoantipyrine and phenol by hydrogen peroxide under the catalytic action of peroxidase (Trinder's reaction) [1,2].



Reagent

Components and Concentrations

Good's buffer	pH 6.7	50 mmol/L
Phenol		5 mmol/L
4-Aminoantipyrine		0.3 mmol/L
Cholesterol esterase	(CHE)	≥ 200 U/L
Cholesterol oxidase	(CHO)	≥ 50 U/L
Peroxidase	(POD)	≥ 3 kU/L

Storage Instructions and Reagent Stability

The reagent is stable up to the end of the indicated month of expiry, if stored at 2 – 8°C, protected from light and contamination is avoided. Do not freeze the reagent!

Warnings and Precautions

- The reagent contains sodium azide (0.95 g/L) as preservative. Do not swallow! Avoid contact with skin and mucous membranes.
- N-acetylcysteine (NAC), acetaminophen and metamizole medication leads to falsely low results in patient samples.
- In very rare cases, samples of patients with gammopathy might give falsified results [8].
- Please refer to the safety data sheets and take the necessary precautions for the use of laboratory reagents. For diagnostic purposes, the results should always be assessed with the patient's medical history, clinical examinations and other findings.
- For professional use only!

Waste Management

Please refer to local legal requirements.

Reagent Preparation

The reagent is ready to use. The bottles are placed directly into the reagent tray.

Specimen

Serum, heparin plasma or EDTA plasma

Stability [3]:

7 days	at	20 – 25°C
7 days	at	4 – 8°C
3 months	at	–20°C

Freeze only once. Discard contaminated specimens.

Calibrators and Controls

For calibration the DiaSys TruCal U calibrator is recommended. The assigned values of the calibrator have been made traceable to the reference method gas chromatography-isotope dilution mass spectrometry (GC-IDMS). For internal quality control DiaSys TruLab N and P or TruLab L controls should be assayed. Each laboratory should establish corrective actions in case of deviations in control recovery.

	Cat. No.	Kit size
TruCal U	5 9100 99 10 063	20 x 3 mL
	5 9100 99 10 064	6 x 3 mL
TruLab N	5 9000 99 10 062	20 x 5 mL
	5 9000 99 10 061	6 x 5 mL
TruLab P	5 9050 99 10 062	20 x 5 mL
	5 9050 99 10 061	6 x 5 mL
TruLab L Level 1	5 9020 99 10 065	3 x 3 mL
TruLab L Level 2	5 9030 99 10 065	3 x 3 mL

Performance Characteristics

Measuring range up to 750 mg/dL (19.4 mmol/L) cholesterol (in case of higher concentrations re-measure samples after manual dilution with NaCl (9 g/L) or use rerun function)	
Limit of detection**	1 mg/dL (0.026 mmol/L) cholesterol
On-board stability	6 weeks
Calibration stability	6 weeks

Interfering substance	Interferences < 10%	Analyte concentration
Ascorbate	up to 6 mg/dL	166 mg/dL (4.29 mmol/L)
Hemoglobin	up to 300 mg/dL	228 mg/dL (5.90 mmol/L)
Bilirubin, conjugated	up to 13 mg/dL	193 mg/dL (4.99 mmol/L)
Bilirubin, unconjugated	up to 15 mg/dL	209 mg/dL (5.41 mmol/L)
Lipemia (triglycerides)	up to 2000 mg/dL	180 mg/dL (4.66 mmol/L)

For further information on interfering substances refer to Young DS [7].

Precision (BX-3010)			
Within run (n=20)	Sample 1	Sample 2	Sample 3
Mean [mg/dL]	82.2	137	286
Mean [mmol/L]	2.13	3.54	7.39
Coefficient of variation [%]	2.02	1.82	1.70
Between run (n=20)	Sample 1	Sample 2	Sample 3
Mean [mg/dL]	142	225	340
Mean [mmol/L]	3.67	5.83	8.79
Coefficient of variation [%]	3.01	2.07	1.49

Method comparison (n=106)	
Test x	Cholesterol FS (BioMajesty 6010C)
Test y	Cholesterol FS (BX-3010)
Slope	1.002
Intercept	–4.04 mg/dL (–0.104 mmol/L)
Coefficient of correlation	0.999

** lowest measurable concentration which can be distinguished from zero mean + 3 SD (n=20) of an analyte free specimen

Conversion factor

Cholesterol [mg/dL] x 0.02586 = Cholesterol [mmol/L]

Reference Range [4]

Desirable	< 200 mg/dL (< 5.2 mmol/L)
Borderline high risk	200 – 240 mg/dL (5.2 – 6.2 mmol/L)
High risk	≥ 240 mg/dL (≥ 6.2 mmol/L)

Each laboratory should check if the reference ranges are transferable to its own patient population and determine own reference ranges if necessary.


Clinical Interpretation

The European Task Force on Coronary Prevention recommends to lower TC concentration to less than 190 mg/dL (5.0 mmol/L) and LDL-cholesterol to less than 115 mg/dL (3.0 mmol/L) [5].

Literature

- Artiss JD, Zak B. Measurement of cholesterol concentration. In: Rifai N, Warnick GR, Dominiczak MH, eds. Handbook of lipoprotein testing. Washington: AACC Press, 1997: p. 99-114.
- Deeg R, Ziegenhorn J. Kinetic enzymatic method for automated determination of total cholesterol in serum. Clin Chem 1983; 29: 1798-802.
- Guder WG, Zawta B et al. The Quality of Diagnostic Samples. 1st ed. Darmstadt: GIT Verlag; 2001. p. 22-3.
- Schaefer EJ, McNamara J. Overview of the diagnosis and treatment of lipid disorders. In: Rifai N, Warnick GR, Dominiczak MH, eds. Handbook of lipoprotein testing. Washington: AACC press, 1997: p. 25-48.
- Recommendation of the Second Joint Task Force of European and other Societies on Coronary Prevention. Prevention of coronary heart disease in clinical practice. Eur Heart J 1998; 19: 1434-503.
- Rifai N, Bachorik PS, Albers JJ. Lipids, lipoproteins and apolipoproteins. In: Burtis CA, Ashwood ER, editors. Tietz Textbook of Clinical Chemistry. 3rd ed. Philadelphia: W.B Saunders Company; 1999. p. 809-61.
- Young DS. Effects of Drugs on Clinical Laboratory Tests. 5th ed. Volume 1 and 2. Washington, DC: The American Association for Clinical Chemistry Press 2000.
- Bakker AJ, Mücke M. Gammopathy interference in clinical chemistry assays: mechanisms, detection and prevention. ClinChemLabMed 2007;45(9):1240-1243.

Manufacturer

 DiaSys Diagnostic Systems GmbH
Alte Strasse 9 65558 Holzheim Germany

Chemistry Parameters 1			Sysmex BX-3010 Chemistry Analyzer Analytical Parameters																						
Method No.	* <input type="text"/>	Method Name	<input type="text" value="CHOL"/>	Reagent Name	Reagent (μL) Water (μL)																				
Print Name	<input type="text" value="Cholesterol"/>	MethodColor		R1	<input type="text" value="CHOL"/> <input type="text" value="135"/>																				
Sample Type	<input type="text" value="Serum"/>			R2	<input type="text" value="Disable"/>																				
Unit	<input type="text" value="mg/dL"/>			Diluent	<input type="text" value="Disable"/>																				
Assay Type	<input type="text" value="End"/>			Sample Ppt. Wash	<input type="text" value="Disable"/>																				
Measuring points		Start	End	Stirring Speed R1	<input type="text" value="Middle"/> R2 <input type="text"/>																				
	1	<input type="text" value="45"/>	- <input type="text" value="46"/>																						
	2	<input type="text" value="Disable"/>	- <input type="text"/>																						
Wave Length				Normal Range																					
	Prim. <input type="text" value="510"/>	Sec. <input type="text" value="700"/>		<table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>No.</th> <th>Normal Range Name</th> <th>Min</th> <th>Max</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>Male-G1</td> <td>*</td> <td>*</td> </tr> <tr> <td>2</td> <td>Male-G2</td> <td>*</td> <td>*</td> </tr> <tr> <td>3</td> <td>Male-G3</td> <td>*</td> <td>*</td> </tr> <tr> <td>4</td> <td>Female-G1</td> <td>*</td> <td>*</td> </tr> </tbody> </table>		No.	Normal Range Name	Min	Max	1	Male-G1	*	*	2	Male-G2	*	*	3	Male-G3	*	*	4	Female-G1	*	*
No.	Normal Range Name	Min	Max																						
1	Male-G1	*	*																						
2	Male-G2	*	*																						
3	Male-G3	*	*																						
4	Female-G1	*	*																						
Normal	Sample Volume (μL)	Diluted Sample (μL)	Diluent (μL)	Technical Range																					
	Low Normal High			(Conc) <input type="text" value="1"/> - <input type="text" value="750"/>																					
<input type="checkbox"/> Diluent	<input type="text" value="0.0"/> < <input type="text" value="1.5"/> < <input type="text" value="0.0"/>	<input type="text"/>	<input type="text"/>	(mAbs/10) <input type="text" value="*"/> - <input type="text" value="*"/>																					
	Rerun (High/Prozone)			Previous Result Comparison (%)	<input type="text" value="*"/> %																				
<input type="checkbox"/> Diluent	<input type="text" value="0.0"/> < <input type="text" value="1.5"/> < <input type="text" value="0.0"/>	<input type="text"/>	<input type="text"/>	Abnormal Range	(Conc) <input type="text" value="*"/> - <input type="text" value="*"/>																				
	Rerun (Low)			Panic Range	(Conc) <input type="text" value="*"/> - <input type="text" value="*"/>																				
<input type="checkbox"/> Diluent	<input type="text" value="0.0"/> < <input type="text" value="1.5"/> < <input type="text" value="0.0"/>	<input type="text"/>	<input type="text"/>	Decimal Point	<input type="text" value="0"/> Profile SI <input type="text" value="Disable"/>																				

*Entered by user

Chemistry Parameters 2		Sysmex BX-3010 Chemistry Analyzer Analytical Parameters	
Method No.	* <input type="text"/>	Method Name	<input type="text" value="CHOL"/>
		Sample	<input type="text" value="Serum"/>
Limit Checks		Blank measurement	
<input checked="" type="checkbox"/> Duplicate Limit	<input type="text" value="50"/> mAbs/10	Blank measurement:	
<input checked="" type="checkbox"/> Sensitivity Limit	<input type="text" value="500"/> mAbs/10	<input type="text" value="Disable reagent blank and C1 blank"/>	
<input checked="" type="checkbox"/> Linearity Limit	<input type="text"/> %	Measurement of Reagent Blank during Run:	
	<input type="text"/> (mAbs/10)/min	<input type="text" value="None"/>	
<input type="checkbox"/> Prozone Limit	<input type="text" value="Higher"/> %	Reagent blank measurement at calibration:	
	<input type="text"/>	<input type="text" value="Reagent blank (No sample)"/>	
	SL1-S <input type="text"/> - SL1-F <input type="text"/>	The number of measurement:	
	SL2-S <input type="text"/> - SL2-F <input type="text"/>	<input type="text" value="Duplicate"/>	
	Sensitivity <input type="text"/> mAbs/10	Reagent blank limit checks:	
<input checked="" type="checkbox"/> Absorbance Limit	Abs. in reaction <input type="text" value="Increase"/>	<input checked="" type="checkbox"/> Duplicate Limit <input type="text" value="20"/> mAbs/10	
	Limit <input type="text" value="25000"/> mAbs/10	Instrument Factor	
		a	<input type="text" value="1.00"/>
		b	<input type="text" value="0.00"/>

Calibration Registration

**Sysmex BX-3010 Chemistry Analyzer
Analytical Parameters**

Method No.

Method Name

Sample Type

Replication

Check Interval

Test without calibration

Calibration Type

Reagent Lot

Calibrator Name


	Conc.	WORK	MASTER	Calibr. Lot No.	<input type="checkbox"/> All
C1	<input type="text" value="0"/>	Automatic entry	Automatic entry	*	
C2	*	Automatic entry	Automatic entry	*	
C3	*				
C4	*				
C5	*				
C6	*				
C7	*				

K C1 Blank
 Reagent Blank for C1

Reagent Lot No.

(R1)
 (R2)

Last

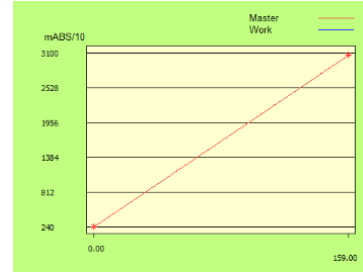

The calibration curve is lot dependent

Reagent blank mAbs/10 Last

Blank mAbs/10 Last

Calibration Curve Conc.

Absorbance mAbs/10

*Entered by user

Cholesterol FS*

Chemistry Code 100 21


Chemistry Parameters		Sysmex BX-4000 Chemistry Analyzer Analytical Parameters																								
Method	* <input type="text"/>	Name	<input type="text" value="CHOL"/>	Reagent Name	Reagent (µL)	Water (µL)																				
Print Name	<input type="text" value="Cholesterol"/>	R1	<input type="text" value="CHOL"/>	<input type="text" value="180"/>	<input type="text"/>	<input type="text"/>																				
Sample	<input type="text" value="Serum"/>	R2	<input checked="" type="checkbox"/> Enable	<input type="text"/>	<input type="text"/>	<input type="text"/>																				
Unit	<input type="text" value="mg/dL"/>																									
Assay Type	<input type="text" value="End"/>	Diluent	<input type="checkbox"/> Enable	<input type="text"/>	<input type="text"/>	<input type="text"/>																				
Measuring points		Start	End	Decimal Points	<input type="text" value="0"/>																					
	<input type="checkbox"/> Enable	1	<input type="text" value="67"/> - <input type="text" value="68"/>																							
		2	<input type="text"/> - <input type="text"/>																							
Wave Length		Normal Range																								
Prim.	<input type="text" value="510"/>	Sec	<input type="checkbox"/> Disable	<input type="text" value="700"/>																						
		<table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>No.</th> <th>Normal Range Name</th> <th>Min</th> <th>Max</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>Male-G1</td> <td>*</td> <td>*</td> </tr> <tr> <td>2</td> <td>Male-G2</td> <td>*</td> <td>*</td> </tr> <tr> <td>3</td> <td>Male-G3</td> <td>*</td> <td>*</td> </tr> <tr> <td>4</td> <td>Female-G1</td> <td>*</td> <td>*</td> </tr> </tbody> </table>				No.	Normal Range Name	Min	Max	1	Male-G1	*	*	2	Male-G2	*	*	3	Male-G3	*	*	4	Female-G1	*	*	
No.	Normal Range Name	Min	Max																							
1	Male-G1	*	*																							
2	Male-G2	*	*																							
3	Male-G3	*	*																							
4	Female-G1	*	*																							
Normal	Sampling	Sample (µL)	Diluent (µL)	Technical Range	(Conc)	<input type="text" value="1"/> - <input type="text" value="750"/>																				
<input type="checkbox"/> Dilution	<input type="text" value="2.0"/>	<input type="text"/>	<input type="text"/>		(mAbs/10)	<input type="text"/>																				
<input type="checkbox"/> Rerun (High/Prozone)	<input type="text"/>	<input type="text"/>	<input type="text"/>			<input type="text"/>																				
<input type="checkbox"/> Dilution	<input type="text" value="2.0"/>	<input type="text"/>	<input type="text"/>																							
<input type="checkbox"/> Rerun (Low)	<input type="text"/>	<input type="text"/>	<input type="text"/>																							
<input type="checkbox"/> Dilution	<input type="text" value="2.0"/>	<input type="text"/>	<input type="text"/>																							
		SPT Wash	<input type="checkbox"/> Enable	Reagent Name	<input type="text"/>																					
		Stirring Speed	R1	<input type="text" value="Middle"/>	R2	<input type="text"/>																				

*Entered by user

Chemistry Parameters		Sysmex BX-4000 Chemistry Analyzer Analytical Parameters	
Method No.	* <input type="text"/>	Name	<input type="text" value="CHOL"/>
		Sample	<input type="text" value="Serum"/>
Limit Checks			
<input checked="" type="checkbox"/> Duplicate Limit	<input type="text" value="50"/>	mAbs/10	
<input checked="" type="checkbox"/> Sensitivity Limit	<input type="text" value="500"/>	mAbs/10	
<input checked="" type="checkbox"/> Linearity Limit	<input type="text"/>	% <input type="text"/> (mAbs/10)/min	
<input type="checkbox"/> Prozone Limit	<input type="text"/>	% <input type="text" value="Upper"/>	
	SL1-S	<input type="text"/> -	SL1-F <input type="text"/>
	SL2-S	<input type="text"/> -	SL2-F <input type="text"/>
	Sensitivity	<input type="text"/>	mAbs/10
<input checked="" type="checkbox"/> Absorbance Limit			
	Reaction	<input type="text" value="Increase"/>	
	Limit	<input type="text" value="25000"/>	mAbs/10
	Blank measurement		
	Blank measurement:	<input type="text" value="Disable reagent blank and S1 blank"/>	
	Measurement of Reagent Blank during Run:	<input type="text" value="None"/>	
	Reagent blank measurement at calibration:	<input type="text" value="Reagent blank (No sample)"/>	
	The number of measurement:	<input type="text" value="Duplicate"/>	
	Reagent blank limit checks:		
<input checked="" type="checkbox"/>	Duplicate Limit	<input type="text" value="20"/>	mAbs/10
	Instrument Factor		
	a	<input type="text" value="1.00"/>	b <input type="text" value="0.00"/>

Cholesterol FS*

Chemistry Code 100 21

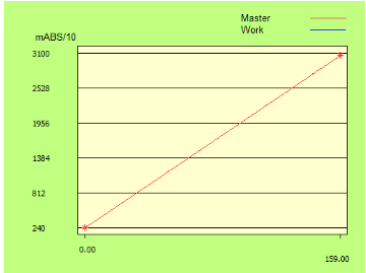Registration Calibration	Sysmex BX-4000 Chemistry Analyzer Analytical Parameters																																
Method <input type="text" value="*"/> Name <input type="text" value="CHOL"/> Sample <input type="text" value="Serum"/> Sampling <input type="text" value="Duplicate"/> Check Interval <input type="text" value="42"/> days Auto <input type="text" value="Change Lot"/> <input type="text" value="Full Calibration"/> Auto Interval <input type="text"/> hours Type <input type="text" value="Linear"/> Lot <input type="text" value="New"/> Material Name <input type="text" value="NaCL/TruCal U"/>	R Lot No. R1 <input type="text" value="*"/> R2 <input type="text" value="*"/> Last <input type="text"/> <div style="text-align: center;">  <p>The calibration curve is lot dependent</p> </div>																																
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th style="width: 5%;">Conc.</th> <th style="width: 20%;">WORK</th> <th style="width: 20%;">MASTER</th> <th style="width: 55%;">Lot No. (S) <input type="checkbox"/> All</th> </tr> </thead> <tbody> <tr><td>S1</td><td><input type="text" value="0"/></td><td><input type="text" value="Automatic entry"/></td><td><input type="text" value="Automatic entry"/></td></tr> <tr><td>S2</td><td><input type="text" value="*"/></td><td><input type="text" value="Automatic entry"/></td><td><input type="text" value="Automatic entry"/></td></tr> <tr><td>S3</td><td><input type="text" value="*"/></td><td><input type="text"/></td><td><input type="text"/></td></tr> <tr><td>S4</td><td><input type="text" value="*"/></td><td><input type="text"/></td><td><input type="text"/></td></tr> <tr><td>S5</td><td><input type="text" value="*"/></td><td><input type="text"/></td><td><input type="text"/></td></tr> <tr><td>S6</td><td><input type="text" value="*"/></td><td><input type="text"/></td><td><input type="text"/></td></tr> <tr><td>S7</td><td><input type="text" value="*"/></td><td><input type="text"/></td><td><input type="text"/></td></tr> </tbody> </table>	Conc.	WORK	MASTER	Lot No. (S) <input type="checkbox"/> All	S1	<input type="text" value="0"/>	<input type="text" value="Automatic entry"/>	<input type="text" value="Automatic entry"/>	S2	<input type="text" value="*"/>	<input type="text" value="Automatic entry"/>	<input type="text" value="Automatic entry"/>	S3	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>	S4	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>	S5	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>	S6	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>	S7	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>	Reagent blank <input type="text"/> mAbs/10 Last <input type="text"/> Blank <input type="text" value="Automatic entry"/> mAbs/10 Last <input type="text"/> Type <input type="text"/> Conc. <input type="text"/> Absorbance <input type="text"/> mAbs/10 <input type="button" value="Recalculation"/>
Conc.	WORK	MASTER	Lot No. (S) <input type="checkbox"/> All																														
S1	<input type="text" value="0"/>	<input type="text" value="Automatic entry"/>	<input type="text" value="Automatic entry"/>																														
S2	<input type="text" value="*"/>	<input type="text" value="Automatic entry"/>	<input type="text" value="Automatic entry"/>																														
S3	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>																														
S4	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>																														
S5	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>																														
S6	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>																														
S7	<input type="text" value="*"/>	<input type="text"/>	<input type="text"/>																														
K <input type="text" value="Automatic entry"/> <input type="checkbox"/> S1 Blank <input type="checkbox"/> Reagent Blank for S1																																	
*Entered by user																																	