

Total bile acids 21 FS*

Order Information

Cat. No.	Kit size
1 2238 99 10 921	 200 (4 x 50)
1 2238 99 10 920	 800 (4 x 200)

Intended Use

Diagnostic reagent for quantitative in vitro determination of total bile acids in human serum on automated respons[®]910.


Summary

Bile acids (BA) are water soluble, amphipathic end products of the cholesterol catabolism which are synthesized in the liver, stored in the gall bladder and secreted in the intestine during digestion [1,2]. Throughout this metabolism, BA change their form from primary via secondary to tertiary BA and their conjugates. Total bile acids (TBA) refer to the sum of all these forms. Serum TBA levels are a sensitive marker of liver function, reflecting hepatic synthesis, secretion and re-absorption [2,3]. Compared to conventional liver screening tests such as ALT or AST, which indicate acute liver damage, the determination of total bile acids allows early detection of liver dysfunction and early treatment and prevention of severe, irreversible liver damage. Once a patient suffers from a liver disease, serum TBA can be used to monitor the treatment response [4-6]. Although TBA levels provide early diagnosis of hepatobiliary deficiencies, they do not allow the differentiation between various diseases. Increased serum TBA levels are associated with several diseases such as acute and chronic hepatitis, intrahepatic cholestasis of pregnancy (ICP), liver sclerosis, cirrhosis, and cancer [2-9]. The determination of TBA levels in pregnant women is considered to be the most important biomarker for diagnosis and monitoring of ICP, also known as obstetric cholestasis [10-12]. ICP is the most common liver disease that occurs during pregnancy; usually during the last 3 months of pregnancy. It is caused by a reversible, hormonally bile secretion disturbance which leads to a restricted bile flow through the gallbladder and in turn, to an accumulation of bile acids in the liver and possibly in the bloodstream [7,13]. Pregnancy-cholestasis is characterized by strong itching (pruritus) [11]. During ICP, TBA levels may rise up to 220 µmol/L [12], leading to an increased risk of fetal distress, premature birth or even stillbirth. TBA concentrations above 40 µmol/L may be fetotoxic [11]. Decreased serum TBA levels are associated with ileal dysfunction, malabsorption, diarrhea or Crohn's disease. In the veterinary field, serum TBA measurements are also of common practice [14].

Method

Enzymatic cycling method

Two reactions are combined in the new generation enzymatic cycling method. In the presence of Thio-NAD, the enzyme 3-α-hydroxysteroid dehydrogenase (3-α-HSD) converts bile acids to 3-ketosteroids and Thio-NADH. The reaction is reversible and 3-α-HSD can convert 3-ketosteroids and NADH to bile acids and NAD. In the presence of excess NADH, the enzyme cycling occurs efficiently and the rate of formation of Thio-NADH is determined by measuring the specific change of absorbance at 405 nm. This cycling reaction leads to significant signal amplification. [15]

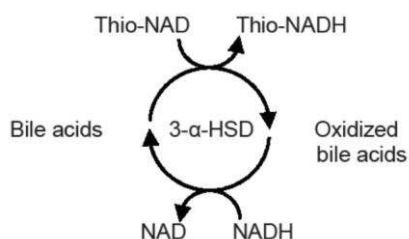

Reagents

Components and Concentrations

R1:	Buffer	
	Thio-NAD	> 0.1 mmol/L
R2:	Buffer	
	3-α-HSD	> 2 kU/L

Storage and Stability

Reagents are stable up to the date of expiry indicated on the kit, if stored at 2 – 8°C and contamination is avoided. Do not freeze and protect from light.

Reagents are temperature-sensitive. Avoid discontinuity of the cold chain.

The in-use stability of the reagent is 15 months.

Warnings and Precautions

1. Reagent 2 contains sodium azide (0.95 g/L) as preservative. Do not swallow! Avoid contact with skin and mucous membranes.
2. Reagent 2 contains material of biological origin. Handle the product as potentially infectious according to universal precautions and good clinical laboratory practice.
3. Postprandial serum TBA levels are generally higher than fasting serum TBA levels. Thus, fasting samples should be used for bile acid determination [3].
4. In very rare cases, samples of patients with gammopathy might give falsified results [16].
5. In case of product malfunction or altered appearance that could affect the performance, contact the manufacturer.
6. Any serious incident related to the product must be reported to the manufacturer and the competent authority of the Member State where the user and/or patient is located.
7. Please refer to the safety data sheets (SDS) and take the necessary precautions for the use of laboratory reagents. For diagnostic purposes, the results should always be assessed with the patient's medical history, clinical examinations and other findings.
8. For professional use only.

Waste Management

Refer to local legal requirements for chemical disposal regulations as stated in the relevant SDS to determine the safe disposal.

Warning: Handle waste as potentially biohazardous material. Dispose of waste according to accepted laboratory instructions and procedures.

Reagent Preparation

The reagents are ready to use. The bottles are placed directly into the reagent rotor.

Materials Required

General laboratory equipment

Specimen

Human serum (fasting > 12h)

Only use suitable tubes or collection containers for specimen collection and preparation.

When using primary tubes, follow the manufacturer's instructions.

Samples from patients under bile acid analogues treatment such as fusidic acid, ursodeoxycholic acid or obeticholic acid are unsuitable for analysis [17].

Stability:

1 day	at	20 – 25°C
1 week	at	2 – 8°C
1 year	at	-20°C

Only freeze once. Discard contaminated specimens.

Calibrators and Controls

DiaSys TruCal TBA is recommended for calibration. Calibrator values have been made traceable to a commercially available measurement procedure. Use DiaSys TruLab N and P for internal quality control. Quality control must be performed after calibration. Control intervals and limits have to be adapted to the individual requirements of each laboratory. Results must be within the defined ranges. Follow the relevant legal requirements and guidelines. Each laboratory should establish corrective action in case of deviations in control recovery.

	Cat. No.	Kit size
TruCal TBA	1 2240 99 10 037	3 x 1 mL
TruLab N	5 9000 99 10 061	6 x 5 mL
	5 9000 99 10 062	20 x 5 mL
TruLab P	5 9050 99 10 061	6 x 5 mL
	5 9050 99 10 062	20 x 5 mL

Performance Characteristics

Measuring range up to 200 µmol/L. In case of higher activities re-measure samples after manual dilution with NaCl solution (9 g/L) or use rerun function.	
Limit of detection**	2 µmol/L
Onboard stability	14 days with chimneys
Calibration stability	7 days with chimneys

Interfering substance	Interferences ≤ 10% up to	Analyte concentration [µmol/L]
Ascorbic acid	100 mg/dL	9.42
	100 mg/dL	24.0
Bilirubin (conjugated)	60 mg/dL	9.37
	60 mg/dL	26.1
Bilirubin (unconjugated)	21 mg/dL	8.99
	35 mg/dL	26.3
Hemoglobin	1000 mg/dL	8.75
	1000 mg/dL	26.5
Lipemia (triglycerides)	600 mg/dL	8.99
	2000 mg/dL	29.0
Sulfapyridine	350 mg/L	8.84
	350 mg/L	28.1
Sulfasalazine	350 mg/L	7.38
	350 mg/L	26.2
Temozolomide	30 mg/L	8.43
	30 mg/L	27.8

For further information on interfering substances refer to Young DS [18,19].

Precision			
Within run (n=20)	Sample 1	Sample 2	Sample 3
Mean [µmol/L]	5.87	11.3	193
CV [%]	2.08	2.48	1.11
Between day (n=20)	Sample 1	Sample 2	Sample 3
Mean [µmol/L]	5.76	11.0	189
CV [%]	2.60	2.35	2.46

Method comparison (n=100)	
Test x	Competitor bile acids (Hitachi 917)
Test y	DiaSys Total bile acids 21 FS (respons [®] 910)
Slope	1.06
Intercept	0.288
Coefficient of correlation	0.996

** according to CLSI document EP17-A2, Vol. 32, No. 8

Reference Range [20,21]

< 10 µmol/L (fasting)

Each laboratory should check if the reference ranges are transferable to its own patient population and determine own reference ranges if necessary.

Literature

- Stamp D and Jenkins G. An overview of bile- acid synthesis, chemistry and function. In: Jenkins GJ, Hardie L, editors. Bile Acids: Toxicology and Bioactivity. Royal Society of Chemistry; 2008. p. 1-13.
- Hofmann AF. The continuing importance of bile acids in liver and intestinal disease. Arch. Intern. Med. 1999;159:2647–2658.
- Dufour DR. Liver Disease. In: Burtis CA, Ashwood ER, and Bruns DE eds. Tietz Textbook of Clinical Chemistry and Molecular Diagnostics. 4th ed. Philadelphia: Elsevier Inc; 2006. p. 1782–1787.
- Shima, T, Tada H, Morimoto M, et al. Serum total bile acid level as a sensitive indicator of hepatic histological improvement in chronic hepatitis C patients responding to interferon treatment. J. gastroenterol. Hepatol. 2000;15: 294-299.
- Barnes S, Gallo GA, Trash DB, et al. Diagnostic value of serum bile acid estimations in liver disease. J Clin Pathol. 1975;28:506-9.
- Skrede S, Solberg HE, Blomhoff JP, et al. Bile acids measured in serum during fasting as a test for liver disease. Clinical Chemistry. 1978;24:1095-1099.
- Pataia V, Dixon PH, Williamson C. Pregnancy and bile acid disorders. Am. J. Physiol. Gastrointest. Liver Physiol. 2017;313: G1–G6.
- Neale G, Lewis B, Weaver V, et al. Serum bile acids in liver disease. Gut. 1971;12:145-152.
- Charach G, Argov O, Geiger K, et al. Diminished bile acids excretion is a risk factor for coronary artery disease: 20-year follow up and long-term outcome. Therap. Adv. Gastroenterol. 2017;11:1-11.
- Egan N et al. Reference standard for serum bile acids in pregnancy. BJOG. 2012;119:493–498.
- Glantz A, Marschall HU, Mattson LA. Intrahepatic cholestasis of pregnancy: relationships between bile acid levels and fetal complication rates. Hepatology. 2004;40:467–74.
- Brites D. Intrahepatic cholestasis of pregnancy: changes in maternal-fetal bile acid balance and improvement by ursodeoxycholic acid. Ann. Hepatol. 2002;1:20–28.
- Ozkan S, Ceylan Y, Ozkan OV, et al. Review of a challenging clinical issue: Intrahepatic cholestasis of pregnancy. World J Gastroenterol. 2015;21:7134–41.
- Schlesinger DP, Rubin SI. Serum bile acids and the assessment of hepatic function in dogs and cats. 1993;34:6.
- Zhang GH, Cong AR, Xu GB, et al. An enzymatic cycling method for the determination of serum total bile acids with recombinant 3α-hydroxysteroid dehydrogenase. Biochem Biophys Res Commun. 2005;326:87-92.
- Bakker AJ, Mücke M. Gammopathy interference in clinical chemistry assays: mechanisms, detection and prevention. Clin Chem Lab Med. 2007;45:1240-3.
- Brown RS. Use of Obeticholic Acid in Patients With Primary Biliary Cholangitis. Gastroenterol Hepatol. 2018;14:654-657.
- Young DS. Effects of Drugs on Clinical Laboratory Tests. 5th ed. Volume 1 and 2. Washington DC: The American Association for Clinical Chemistry Press; 2000.
- Young DS. Effects on Clinical Laboratory Tests - Drugs Disease, Herbs & Natural Products [Internet]. AACC Press and John Wiley and Sons, Inc; 2020 [cited 2020 Sept]. Available from: <https://clinf.wiley.com/aaccweb/aacc/>.
- Luo L, Aubrecht J, Li D, Warner RL, et al. Assessment of serum bile acid profiles as biomarkers of liver injury and liver disease in humans. PLoS One. 2018;13.
- Jahnel J, Zöhrer E, Scharnagel H, et al. Reference ranges of serum bile acids in children and adolescents. Clin Chem Lab Med. 2015;53:1807-13.

Additions and/or changes in the document are highlighted in grey. For deletions, please refer to the customer information for the corresponding edition number of the package inserts.

respons[®]910



DiaSys Diagnostic Systems GmbH
Alte Strasse 9 65558 Holzheim
Germany
www.diasys-diagnostics.com

* Fluid Stable

Total bile acids 21 FS

Application for serum samples

This application was set up and evaluated by DiaSys. It is based on the standard equipment at that time and does not apply to any equipment modifications undertaken by unqualified personnel.

Identification	
This method is usable for analysis:	Yes
Twin reaction:	No
Name:	TBA
Shortcut:	
Reagent barcode reference:	071
Host reference:	071

Technic	
Type:	Linear kinetic
First reagent:[μ L]	180
Blank reagent	Yes
Sensitive to light	
Second reagent:[μ L]	60
Blank reagent	No
Sensitive to light	
Main wavelength:[nm]	405
Secondary wavelength:[nm]	600
Polychromatic factor:	1.0000
1 st reading time [min:sec]	05:48
Last reading time [min:sec]	10:00
Reaction way:	Increasing
Linear Kinetics	
Substrate depletion: Absorbance limit	1.3500
Linearity: Maximum deviation [%]	
Fixed Time Kinetics	
Substrate depletion: Absorbance limit	
Endpoint	
Stability: Largest remaining slope	
Prozone Limit [%]	

Reagents	
Decimals	
Units	

Sample	
Diluent	DIL A (NaCl)
Hemolysis:	
Agent [μ L]	0 (no hemolysis)
Cleaner	
Sample [μ L]	0
Technical limits	
Concentration technical limits-Lower	2.0000
Concentration technical limits-Upper	200.0000
SERUM	
Normal volume [μ L]	4.0
Normal dilution (factor)	1
Below normal volume [μ L]	
Below normal dilution (factor)	
Above normal volume [μ L]	
Above normal dilution (factor)	
URINE	
Normal volume [μ L]	4.0
Normal dilution (factor)	1
Below normal volume [μ L]	
Below normal dilution (factor)	
Above normal volume [μ L]	
Above normal dilution (factor)	
PLASMA	
Normal volume [μ L]	4.0
Normal dilution (factor)	1
Below normal volume [μ L]	
Below normal dilution (factor)	
Above normal volume [μ L]	
Above normal dilution (factor)	
CSF	
Normal volume [μ L]	4.0
Normal dilution (factor)	1
Below normal volume [μ L]	
Below normal dilution (factor)	
Above normal volume [μ L]	
Above normal dilution (factor)	
Whole blood	
Normal volume [μ L]	4.0
Normal dilution (factor)	1
Below normal volume [μ L]	
Below normal dilution (factor)	
Above normal volume [μ L]	
Above normal dilution (factor)	

Results	
Decimals	2
Units	μ mol/L
Correlation factor-Offset	0.0000
Correlation factor-Slope	1.0000

Range	
Gender	All
Age	
SERUM	>= <=10.00
URINE	
PLASMA	
CSF	
Whole blood	
Gender	
Age	
SERUM	
URINE	
PLASMA	
CSF	
Whole blood	

Contaminants	
Please refer to r910 Carryover Pair Table	

Calibrators details	
Calibrator list	Concentration
Cal. 1/Blank	0
Cal. 2	*
Cal. 3	
Cal. 4	
Cal. 5	
Cal. 6	
	Max delta abs.
Cal. 1	0.1
Cal. 2	0.1
Cal. 3	
Cal. 4	
Cal. 5	
Cal. 6	
Drift limit [%]	0.80

Calculations	
Model	X
Degree	1

* Enter calibrator value